

## A novel small-angle neutron scattering detector geometry. Corrigendum

Kalliopi Kanaki,<sup>a\*</sup> Andrew Jackson,<sup>a</sup> Richard Hall-Wilton,<sup>a</sup> Francesco Piscitelli,<sup>b</sup> Oliver Kirstein<sup>a</sup> and Ken H. Andersen<sup>a</sup>

<sup>a</sup>European Spallation Source ESS AB, PO Box 176, 22 100 Lund, Sweden, and

<sup>b</sup>Institut Laue–Langevin, Grenoble, France. Correspondence e-mail: kalliopi.kanaki@ess.se

Errors in the paper by Kanaki, Jackson, Hall-Wilton, Piscitelli, Kirstein & Andersen [*J. Appl. Cryst.* (2013), **46**, 1031–1037] are corrected.

In equation (5) of Kanaki *et al.* (2013), a factor of 2 is missing from the wavelength contribution to the  $Q$  resolution. The correct equation is

$$\delta Q = \left\{ \left[ \frac{2\pi \cos(\theta/2)}{\lambda} \delta\theta \right]^2 + \left[ \frac{4\pi \sin(\theta/2)}{\lambda^2} \delta\lambda \right]^2 \right\}^{1/2}. \quad (1)$$


Figs. 12 and 13 of Kanaki *et al.* (2013) are updated as Figs. 1 and 2 of the current article to reflect the correction.

In equation (6) of Kanaki *et al.* (2013), the brackets are missing a square root. The correct version is


$$\delta\lambda = 3956 \left( \frac{\delta t^2}{L^2} + \frac{t^2 \delta L^2}{L^4} \right)^{1/2}. \quad (2)$$

### References

Kanaki, K., Jackson, A., Hall-Wilton, R., Piscitelli, F., Kirstein, O. & Andersen, K. H. (2013). *J. Appl. Cryst.* **46**, 1031–1037.

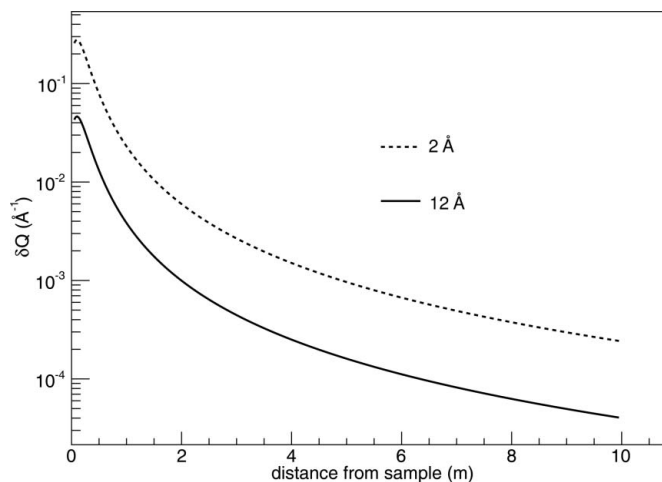

**Figure 1**  
 $Q$  resolution for a 10 m-long and 0.5 m-wide tube detector, as a function of distance from the sample.

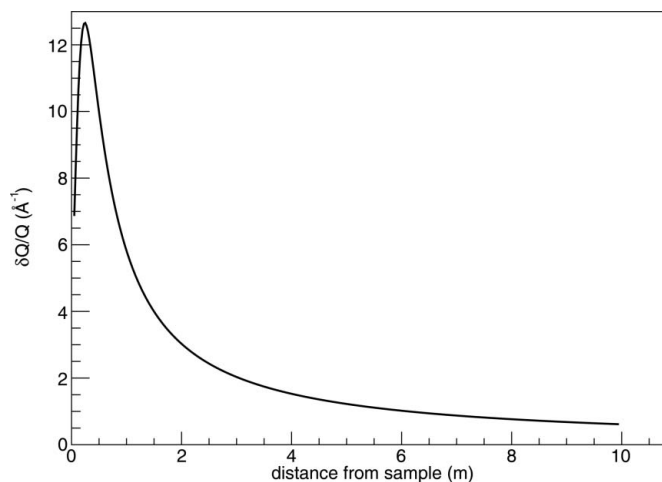

**Figure 2**  
Normalized  $Q$  resolution for a 10 m-long and 0.5 m-wide tube detector, as a function of distance from the sample.